

FIG.1

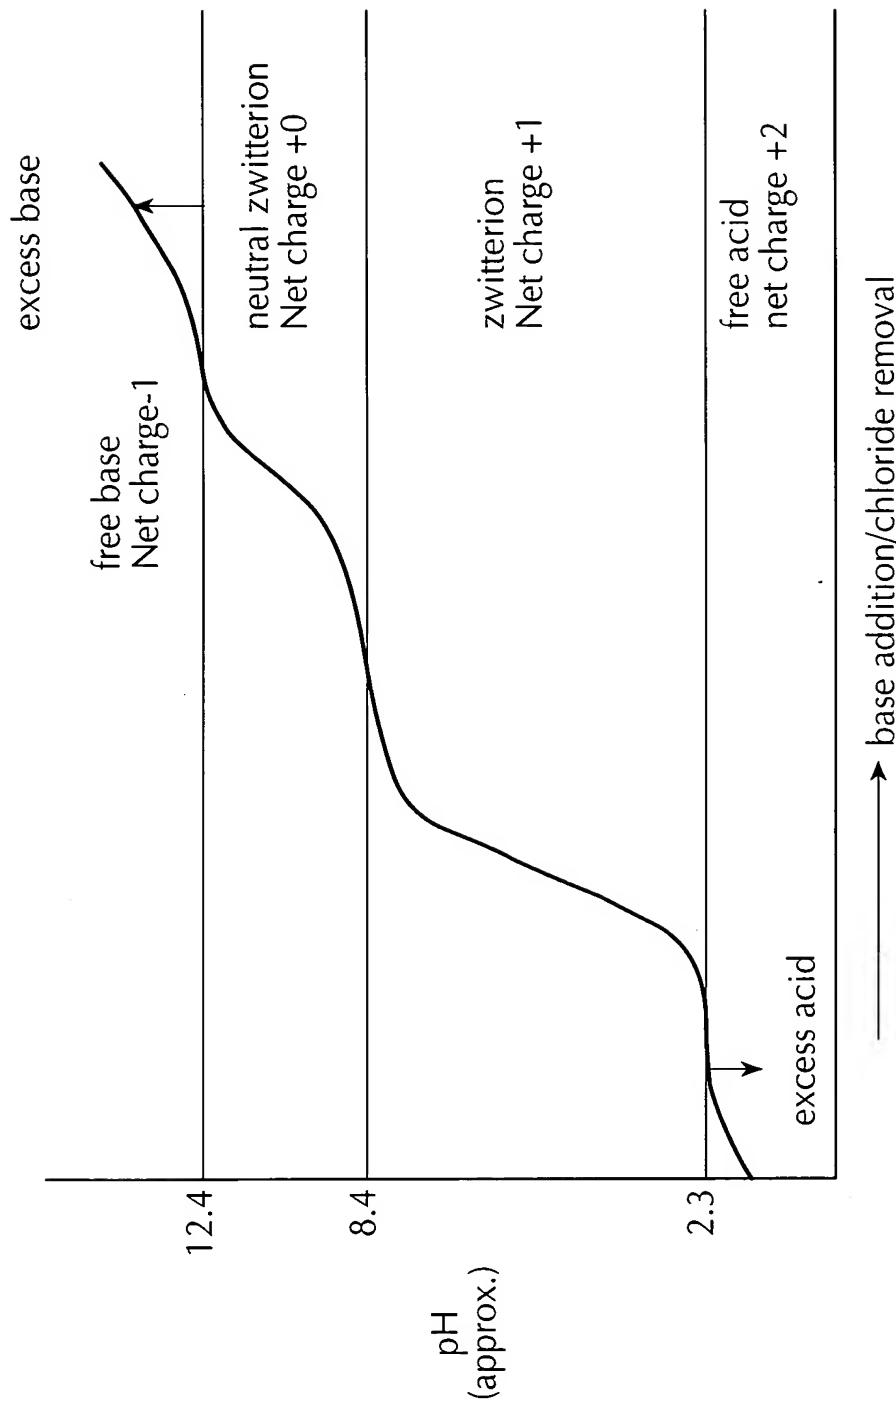


FIG.2

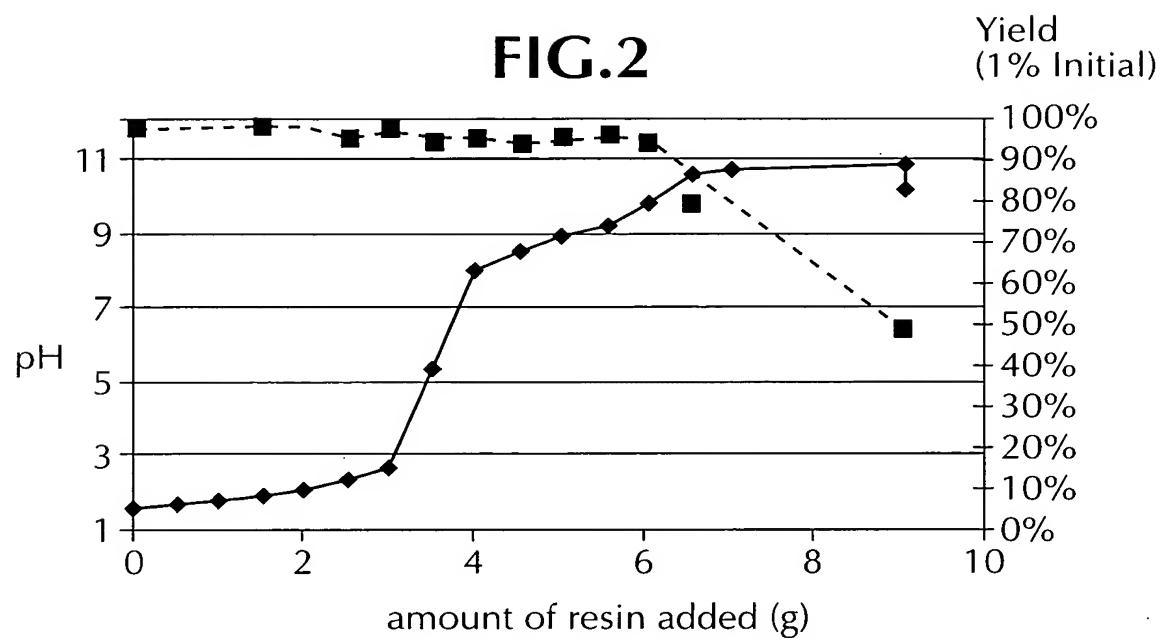


FIG. 3

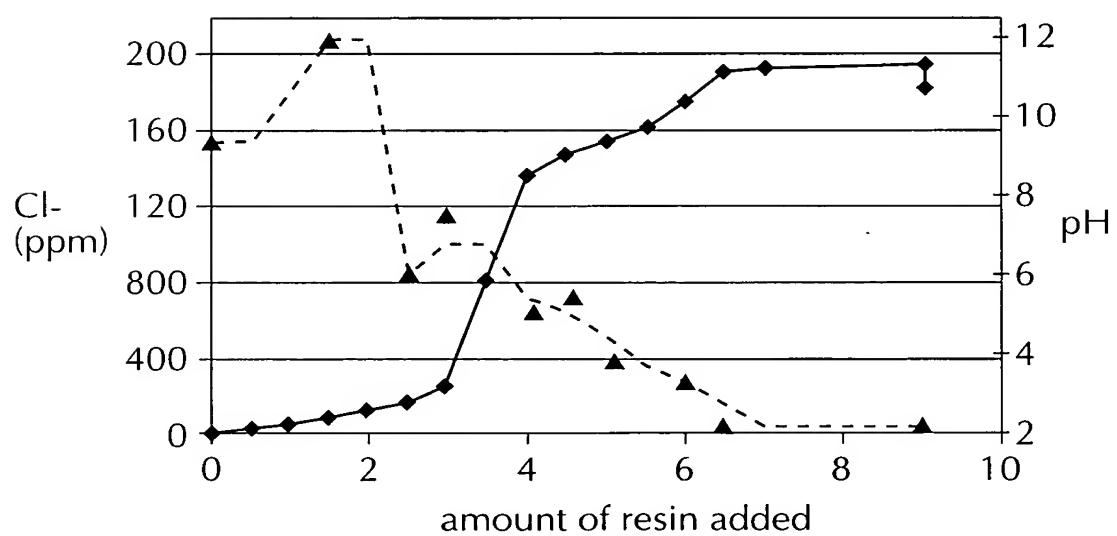


FIG. 4

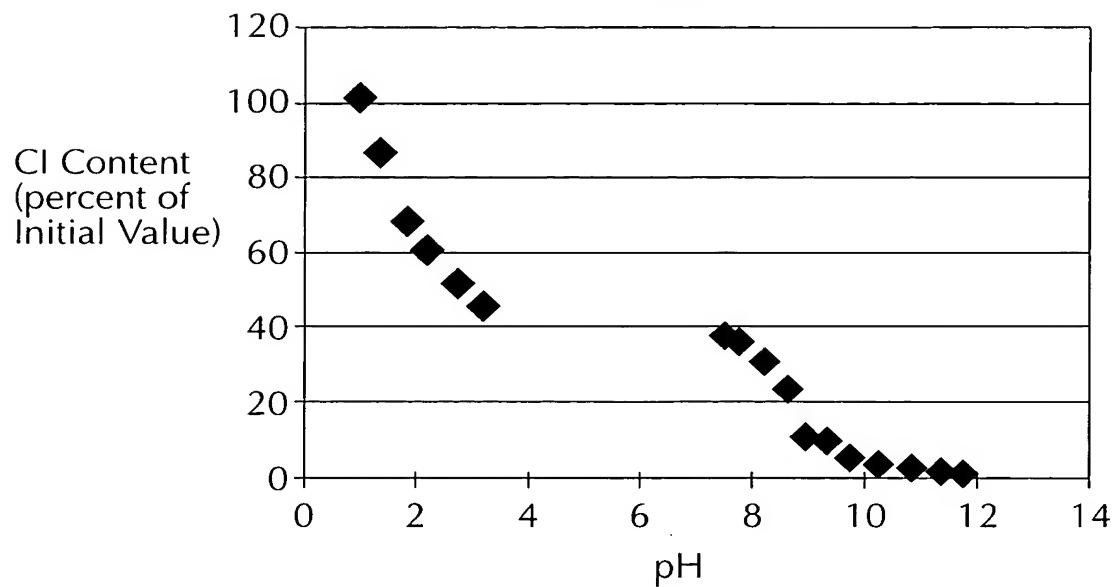


FIG. 5

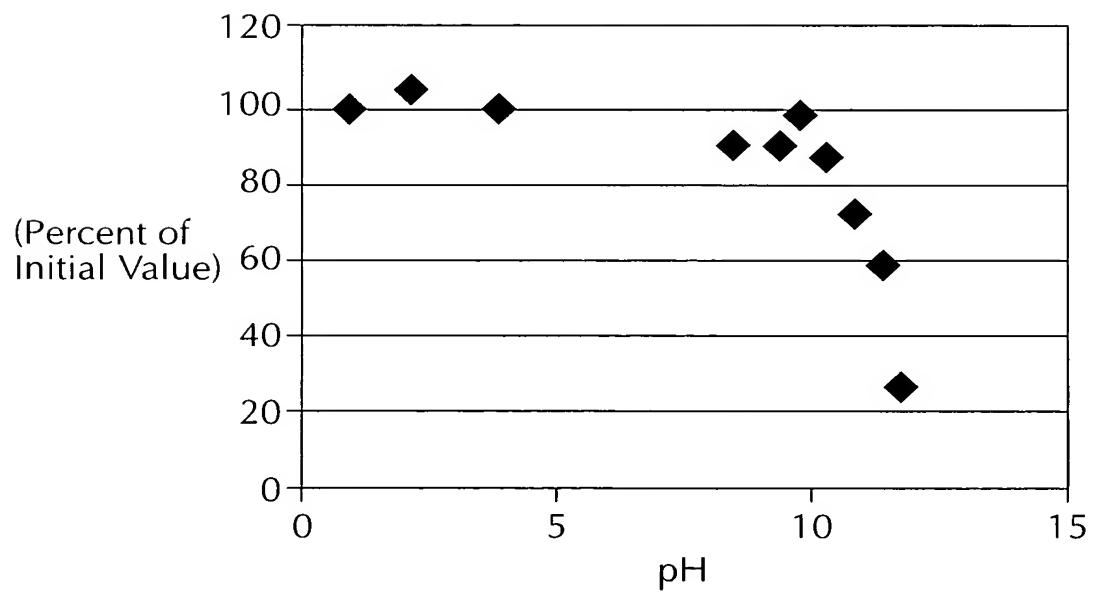


FIG. 6

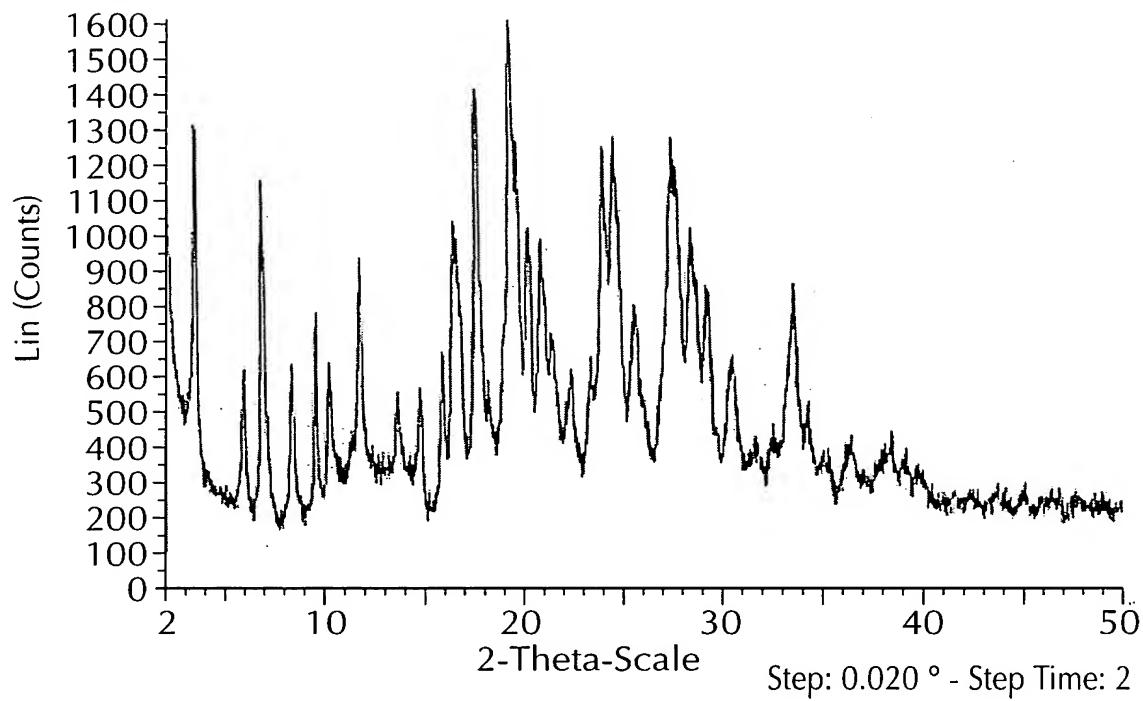


FIG. 7

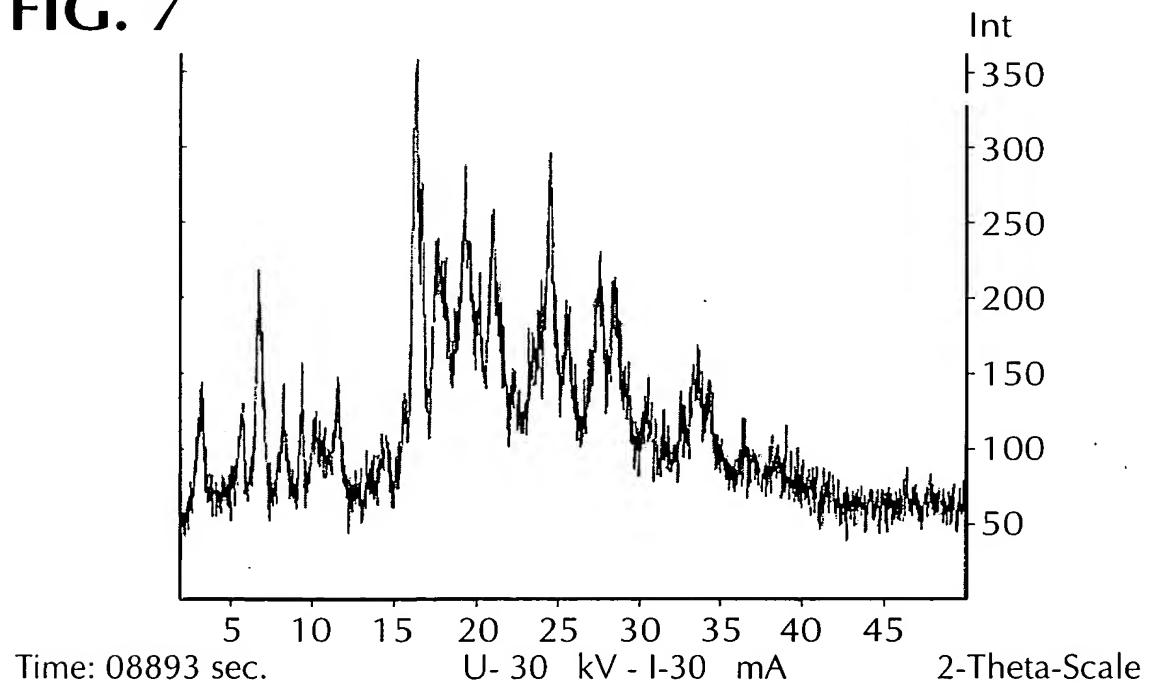


FIG. 8

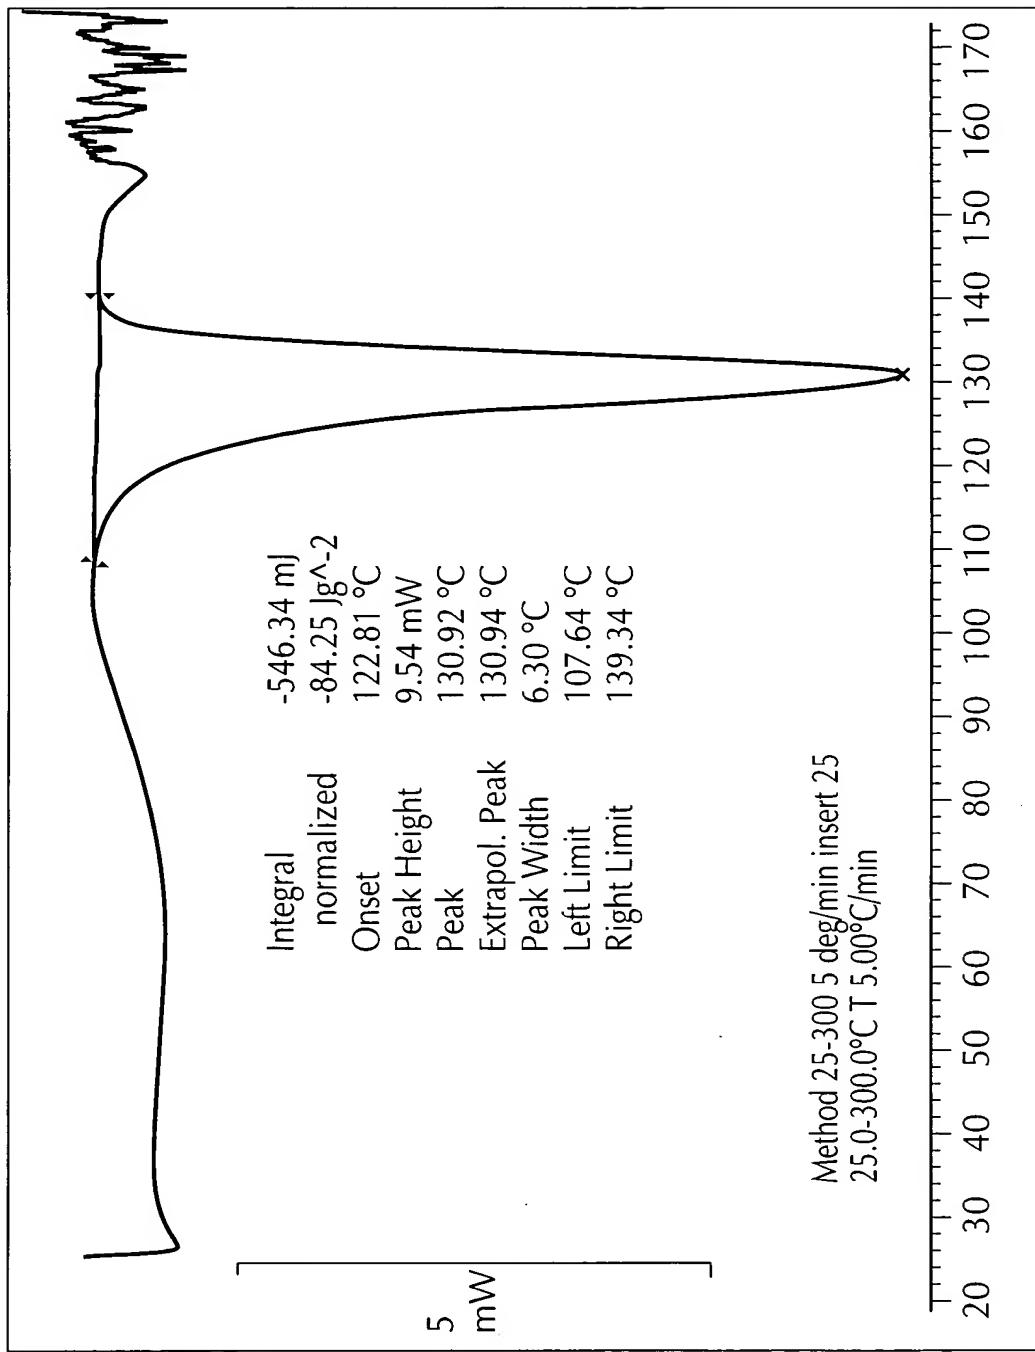


FIG. 9

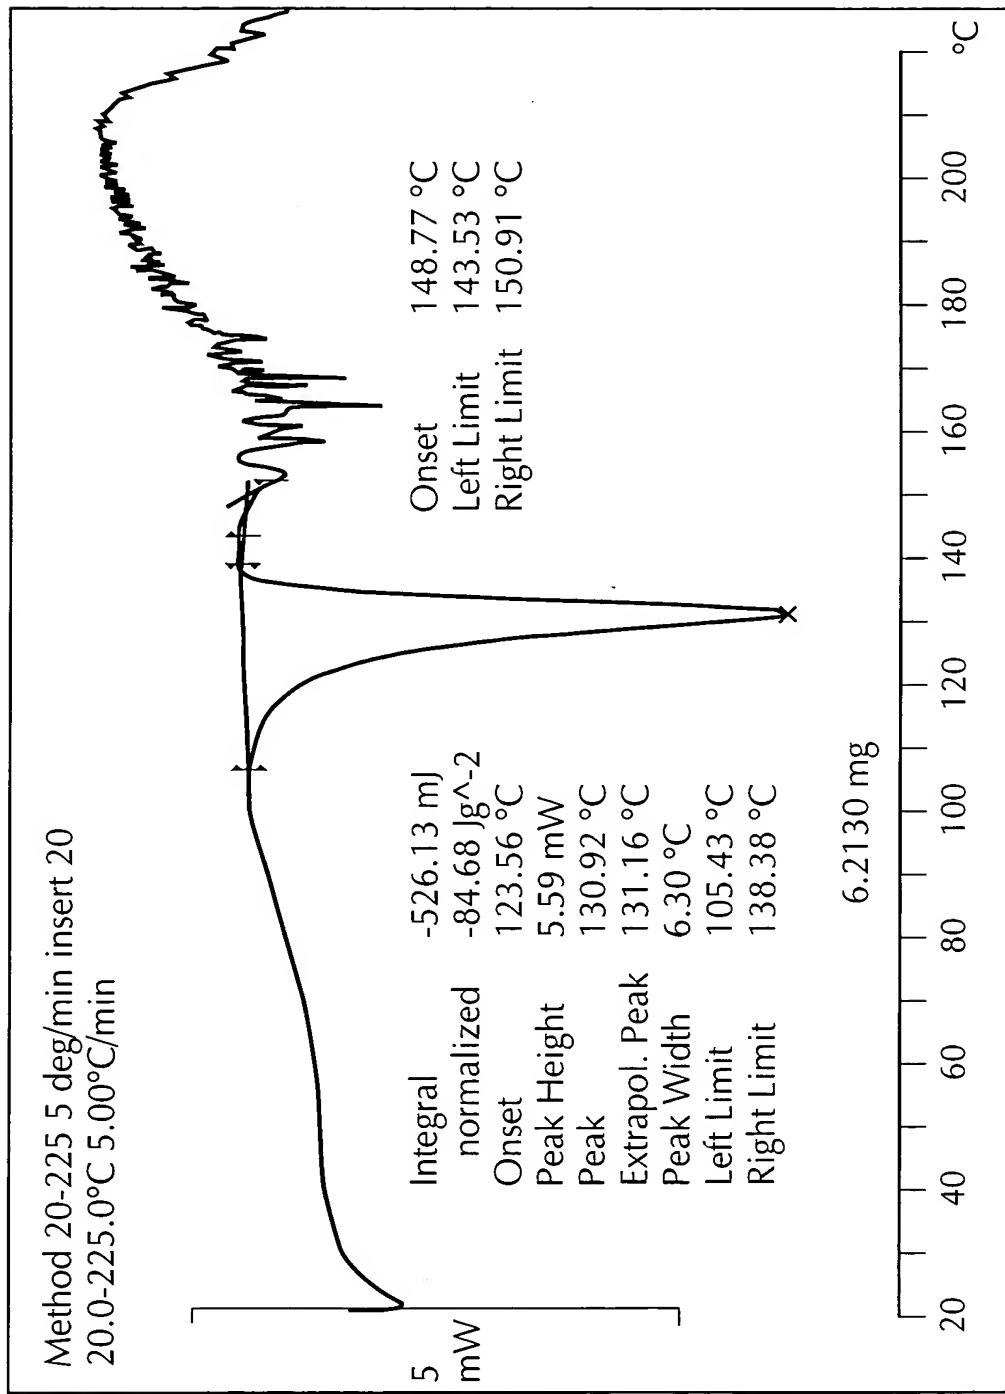


FIG. 10

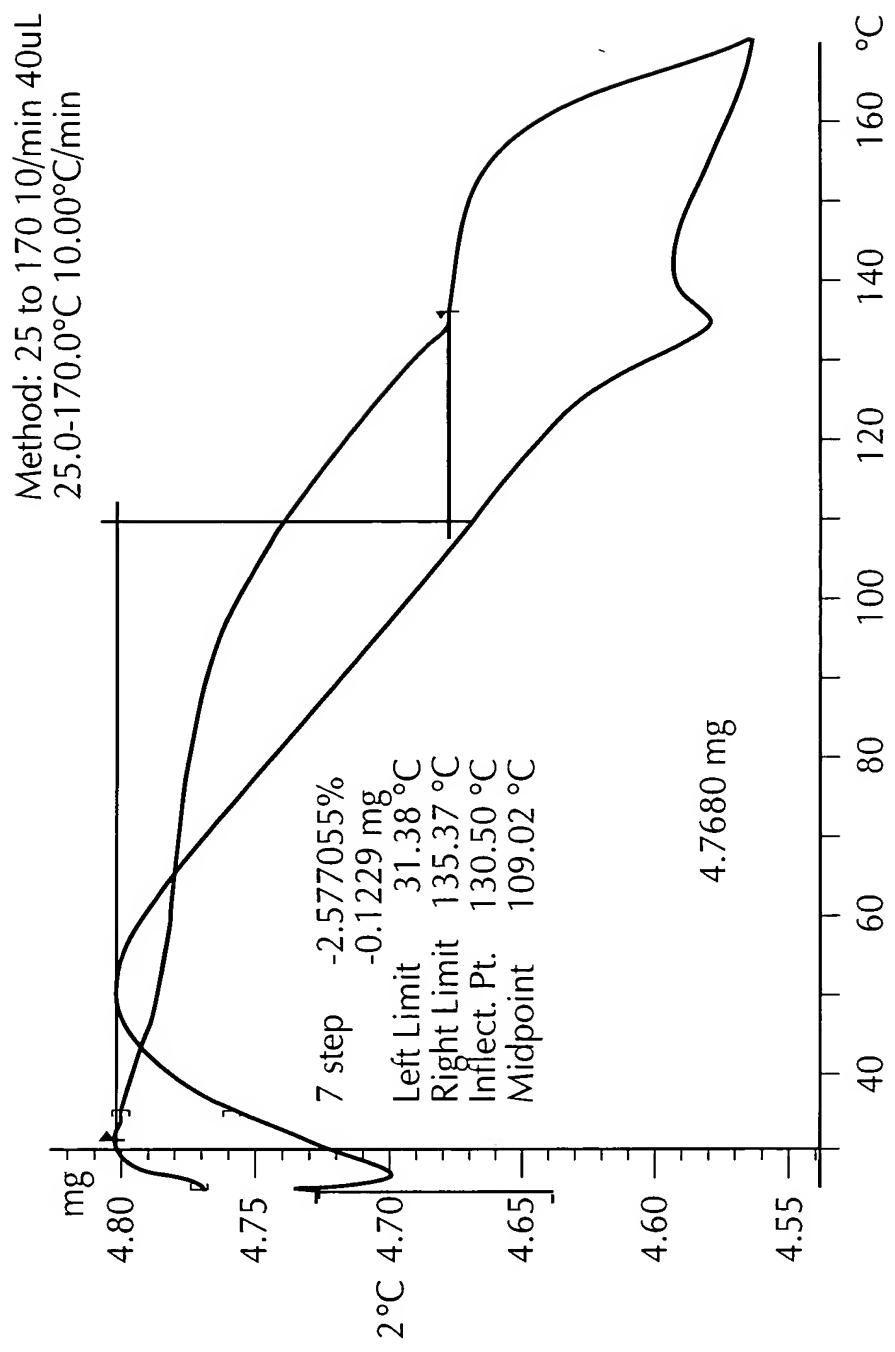


FIG.11

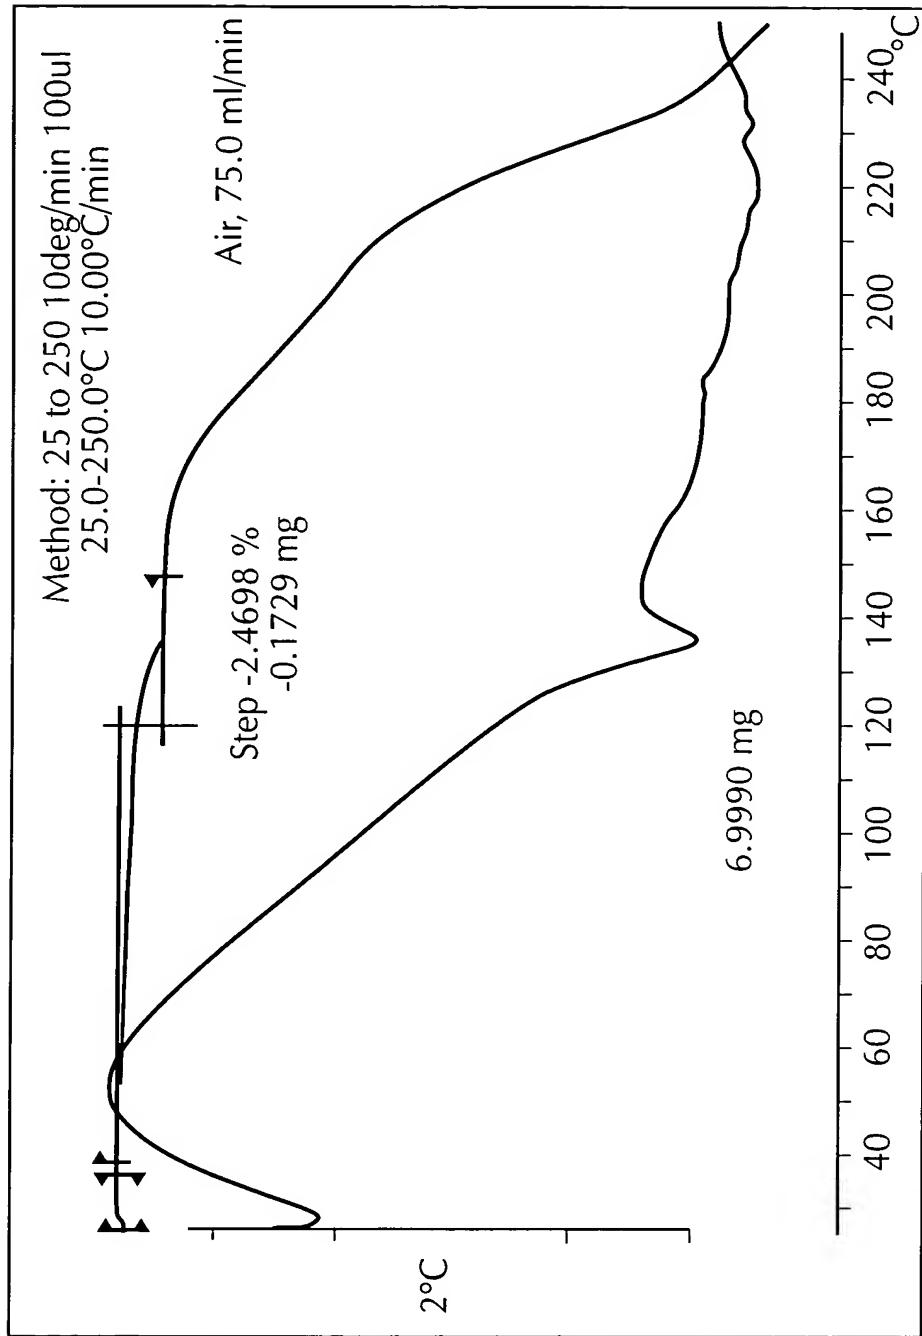


FIG. 12

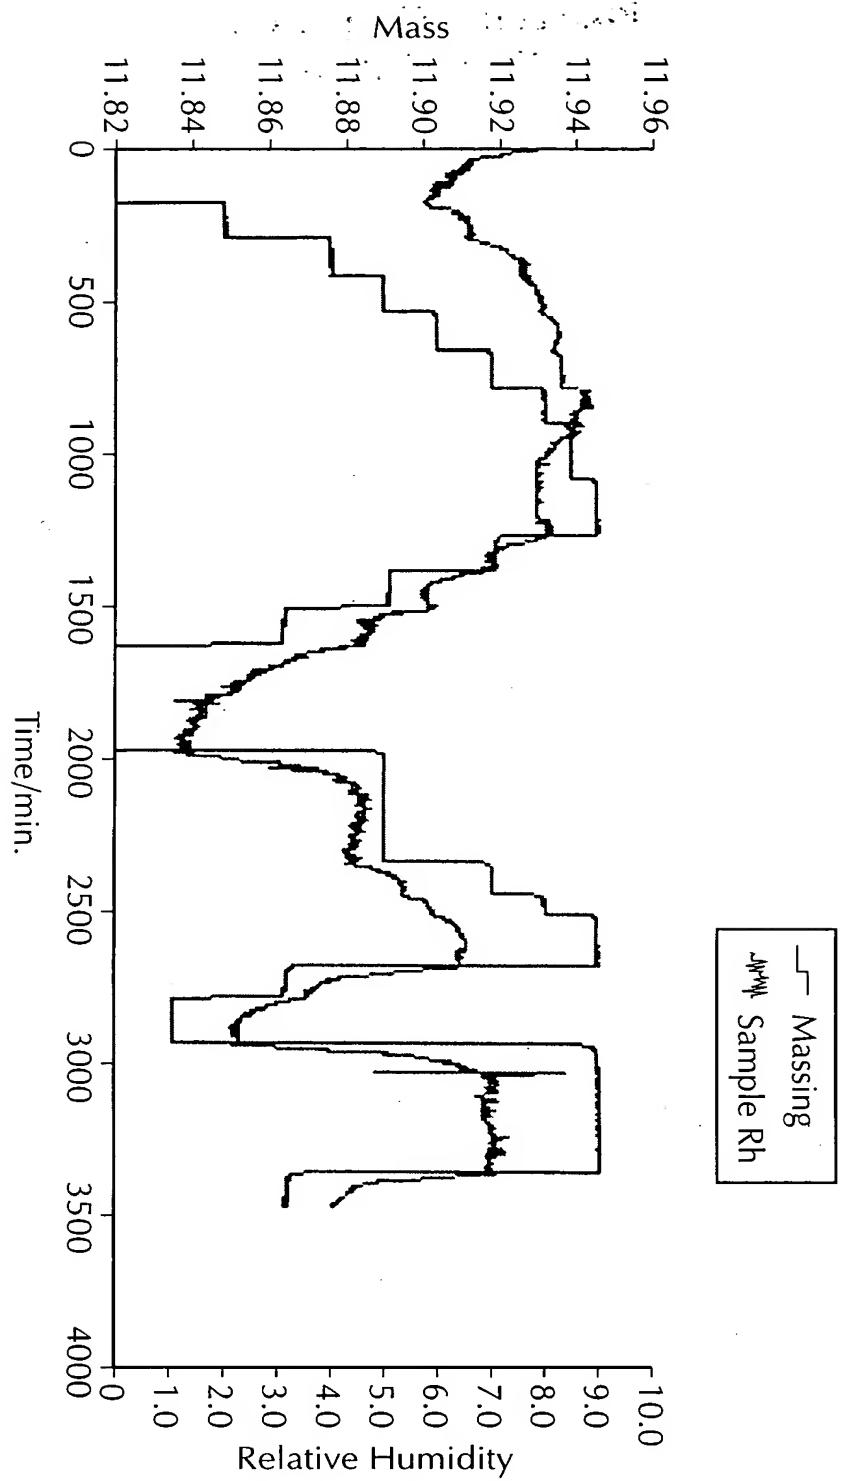


FIG. 13

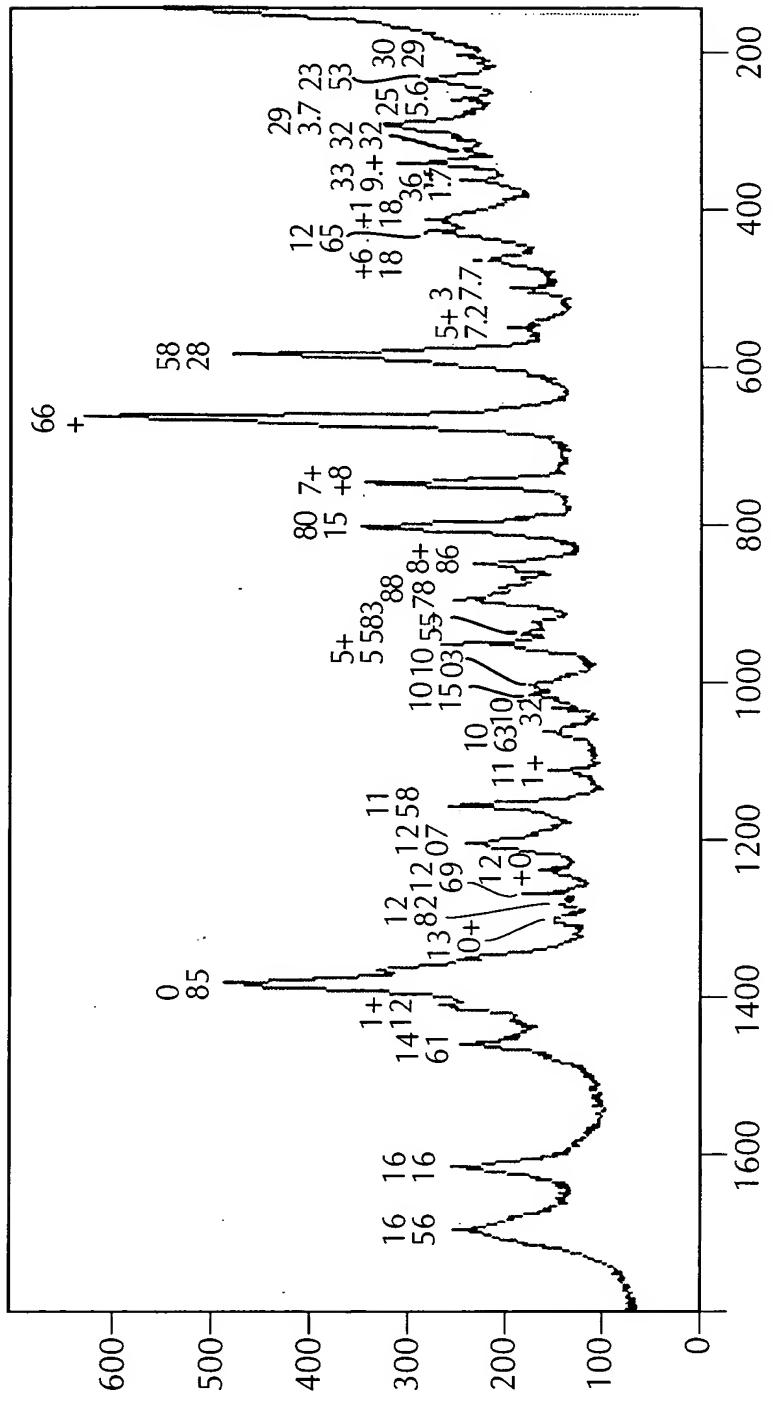


FIG. 14

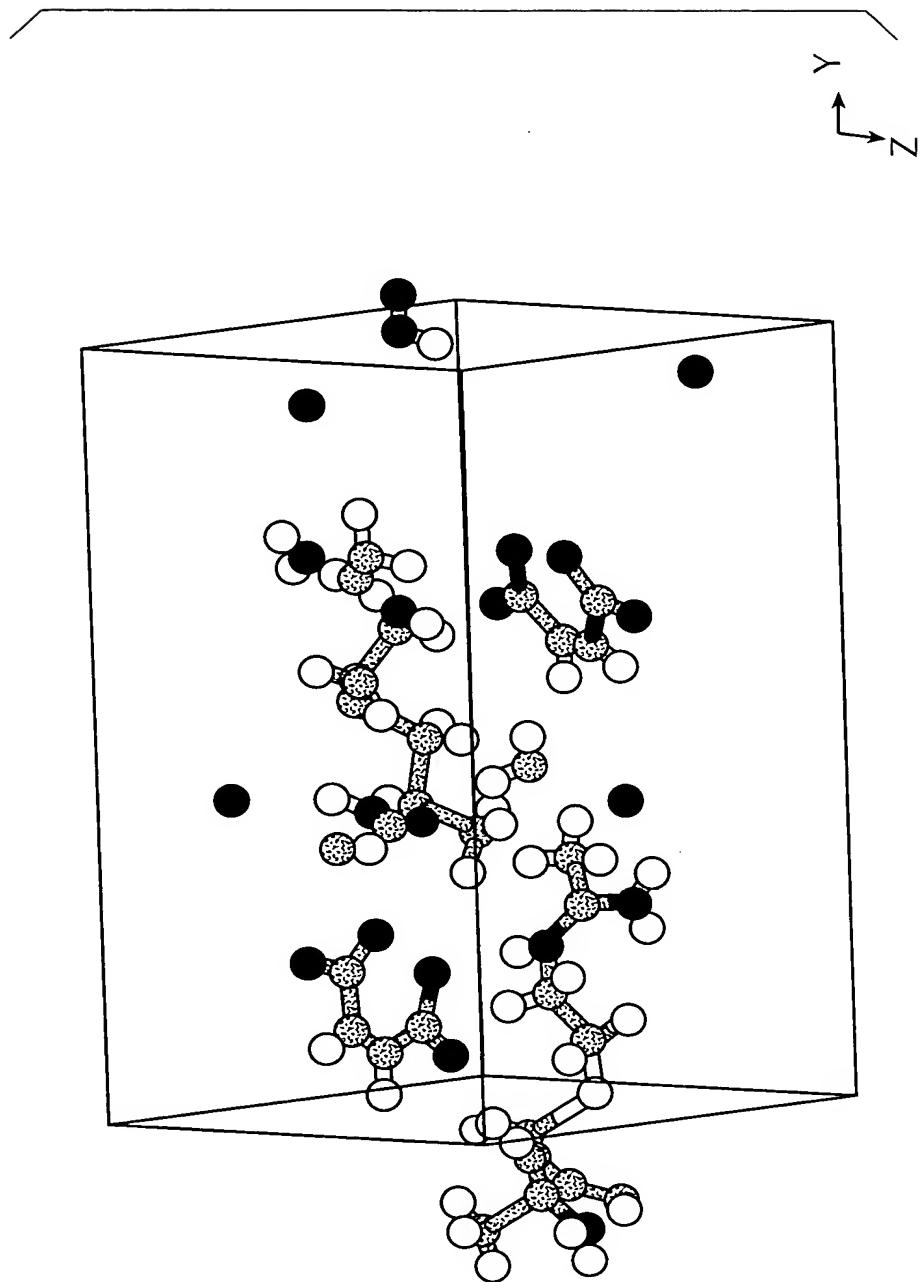


FIG. 15

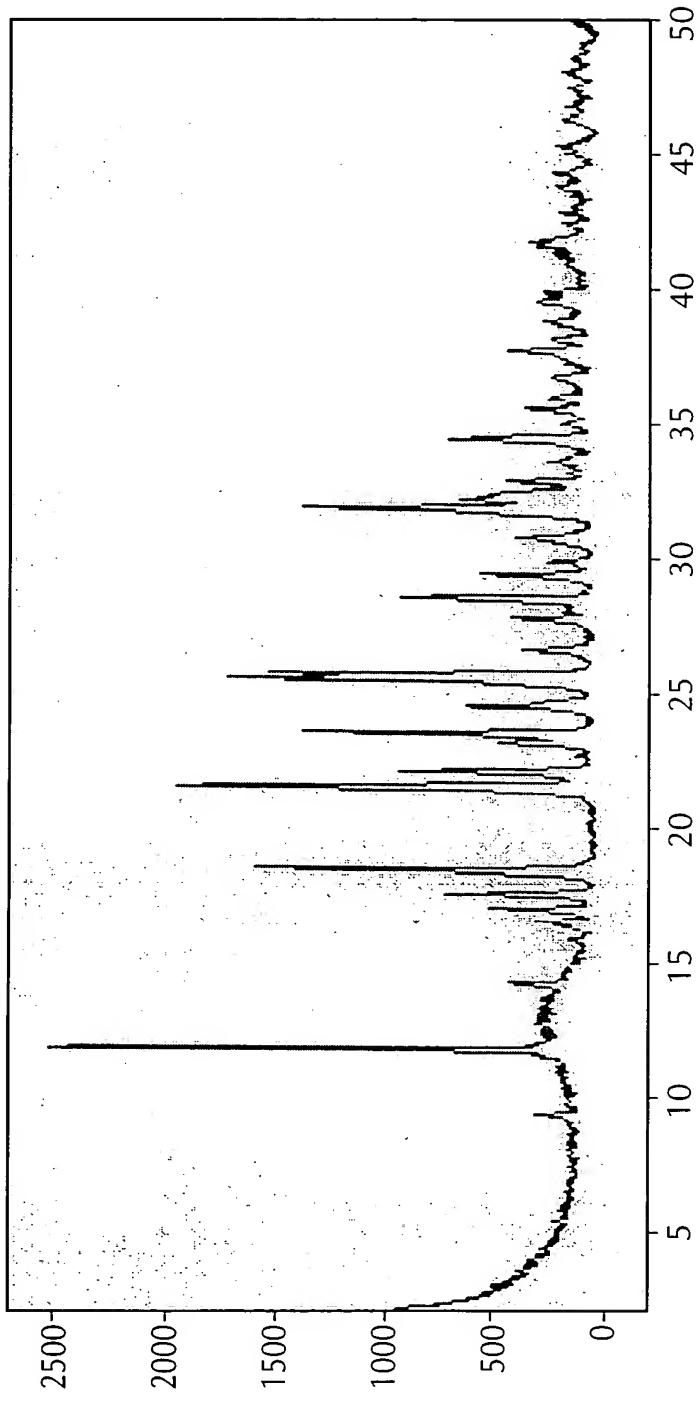


FIG. 16

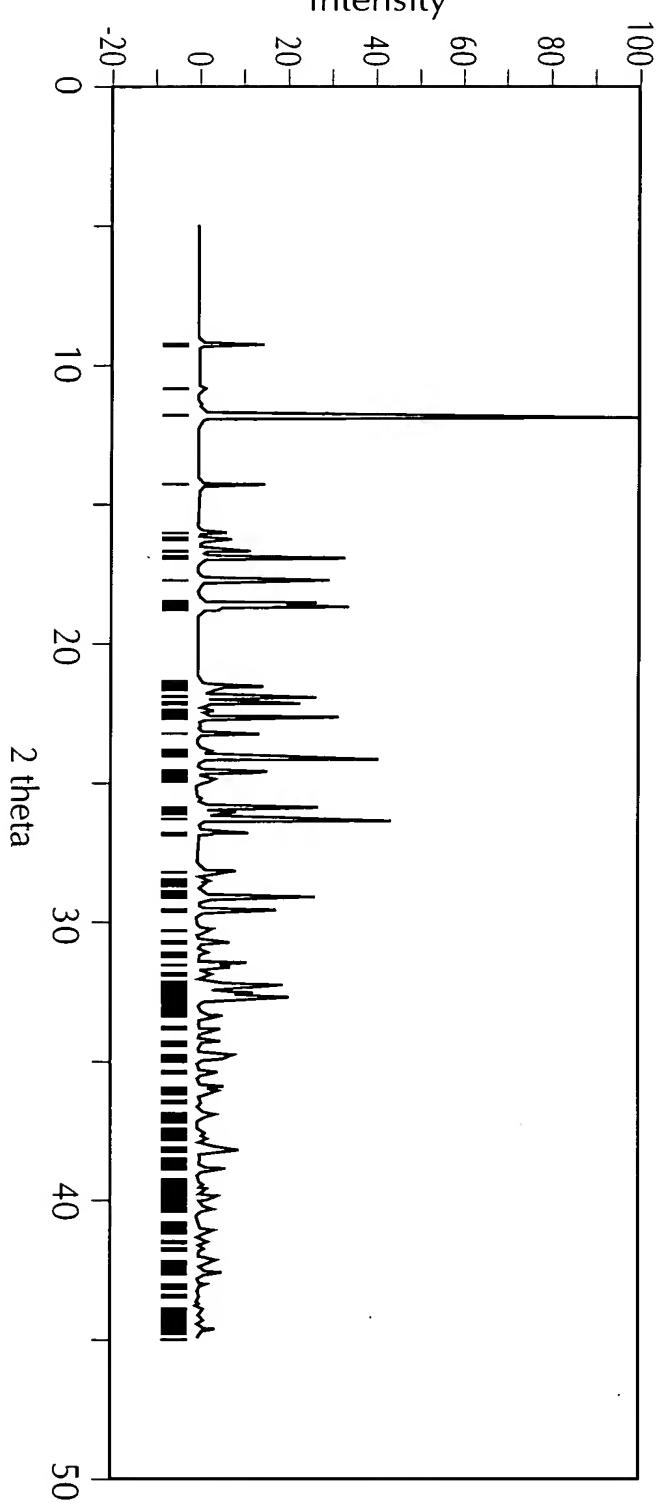


FIG. 17

sealed and pin pricked


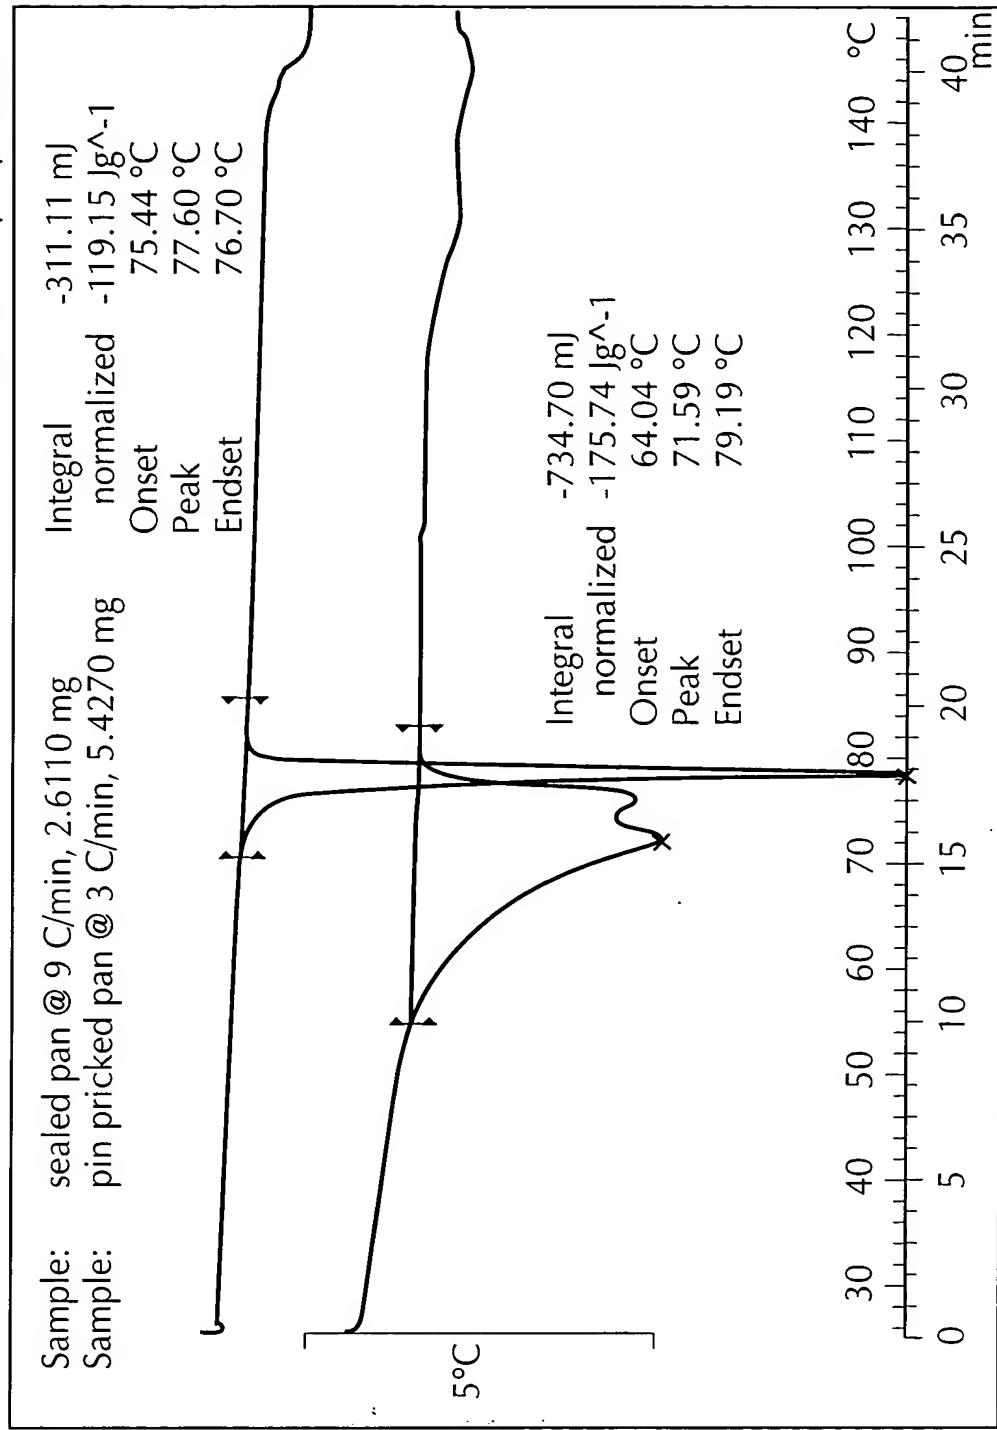


FIG. 18

Sample: 9.7530 mg

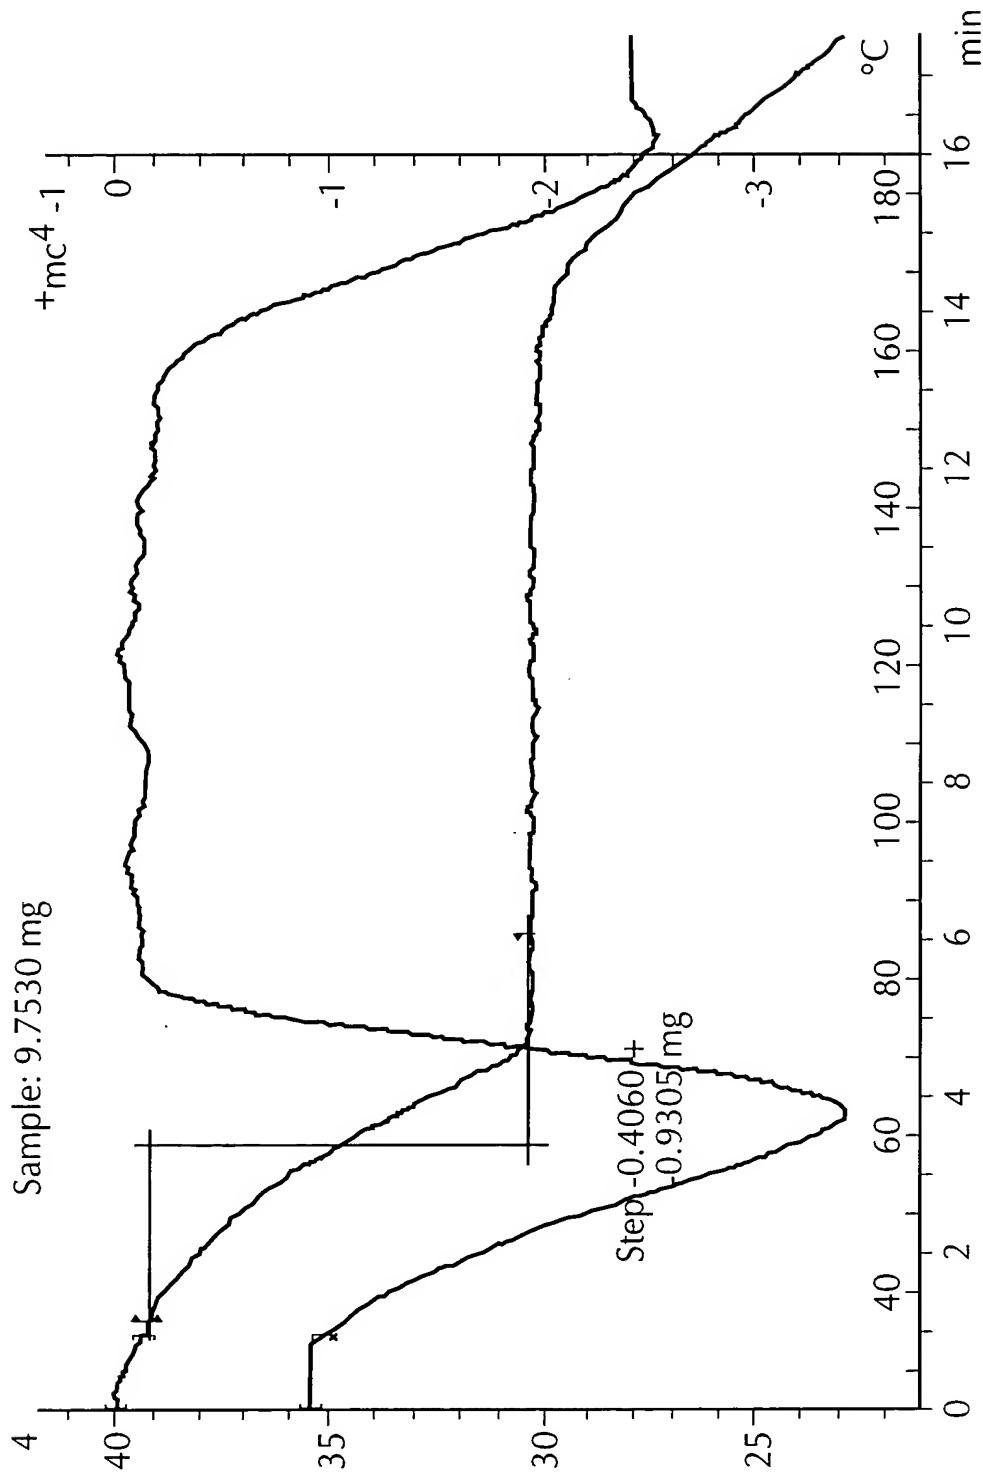

METTLER TOLEDO STAR* System

FIG. 19

